

# MJ/MJH-Series

## Pulse Meter Instructions



**General Information**

General Information .....Page 3  
Specifications .....Page 3  
Pulse Rates .....Page 4

**Installation and Operation**

Position .....Page 4  
Couplings.....Page 4  
Connections.....Page 4  
Pulse Output.....Page 5  
Moving the Magnetic Pointer.....Page 5  
Setting Pulse Rate .....Page 5  
Sample Set Up .....Page 6  
Special Configurations.....Page 6  
Reading Meter .....Page 6

**Maintenance**

Inlet Strainer .....Page 6  
Calibration .....Page 6  
Internal Parts Replacement.....Back

**MJ/MJH-Series** meters use the multi-jet principle, which has been an internationally-accepted standard for many years. This type of meter is known for its wide range, simplicity, and accuracy in low-quality water. The impeller is centered in a ring of jets, with inlet jets on one level and outlet jets on another. A gear train drives the register totalizer dials. For pulse output, one of the pointers is replaced by a magnet, which is detected by an encapsulated sensor attached to the outside of the lens. Pulse rate is determined by the dial on which the magnet is placed, and by the number of sensors (single or double).

MJE (cold water) and MJHE (hot water) meters use a solid-state, long-lasting Hall-effect sensor, which requires power. They are suited for use with Seametrics controls and metering pumps (LMI for instance) that have sensor power.

MJR (cold water) and MJHR (hot water) meters use a reed switch. They provide a dry contact closure and do not require power.

MJT (cold water) and MJHT (hot water) meters do not have a sensor, and they totalize only.

Changing the pulse rate requires no special tools and can be done in the field.

**Specifications\***

<b>Power</b>	6 mA at 12 Vdc				
<b>Temperature</b>	<b>Cold Water</b>	105° F (40° C) max			
	<b>Hot Water</b>	194° F (90° C) max			
<b>Pressure</b>	150 psi operating (10.3 Bar)				
<b>Materials</b>	<b>Body</b>	Cast broze, epoxy powder coated inside and out			
	<b>Internals</b>	Engineered thermoplastic			
	<b>Magnet</b>	Alnico			
<b>Accuracy</b>	± 1.5% of reading				
<b>Pulse Output</b>		<b>MJE/MJHE</b>	<b>MJR/MJHR</b>	<b>MJT/MJHT</b>	
	<b>Sensor</b>	Hall-effect device	Reed switch	Totalizer only	
	<b>Max Current</b>	20 mA	20 mA	n/a	
	<b>Max Voltage</b>	24 Vdc	24 Vdc or Vac	n/a	
<b>Cable Length</b>	12' (3.6 m) standard (2000' maximum run)				
<b>Flow Rates (GPM)**</b>		<b>3/4"</b>	<b>1"</b>	<b>1 1/2"</b>	<b>2"</b>
	<b>Minimum</b>	0.22	0.44	0.88	1.98
	<b>Maximum</b>	22	52	88	132

\*Specifications subject to change • Please consult our website for current data ([www.seametrics.com](http://www.seametrics.com)).

\*\* **Caution:** Excessive flow can cause breakage. Do not exceed recommended maximums.

**Pulse Rates**

	3/4"	1"	1 1/2"	2"
<b>Pulses per Gallon</b>	20* 10 4† 2* 1	4† 2* 1	4† 2* 1	4† 2* 1
<b>Gallons per Pulse</b>	1 5* 10 50* 100	1 5* 10 50* 100	1 5* 10 50* 100	1 5* 10 50* 100
<b>Cubic Feet per Pulse</b>	1 5* 10	1 5* 10	1 5* 10	1 5* 10
<b>Pulses per Cubic Meter</b>	1 10 100	1 10 100	1 10 100	1 10 100
<b>Liters per Pulse</b>	1 10 100	1 10 100	1 10 100	1 10 100

\*MJR/MJHR dual reed switch meters only  
 †MJR/MJHR single reed switch meters only

**Positions**

MJ/MJH-Series meters should be installed horizontally with the register up. Vertical mounting will result in some degree of under-measurement and shortened life of the bearings and may void warranty. No upstream straight pipe is required





**Caution:** These water meters are not recommended for installation in uninsulated suspended ceilings where freezing is possible, or in any overhead indoor piping configuration where leakage may cause damage.

**Couplings**

Male NPT threaded couplings are included with each meter. The threads on the end of the meter are IPS straight threads one size bigger than the meter size. Though it is possible to thread a standard pipe coupling directly onto the meter for close coupling, the included couplings are much preferable because they provide a union connection for meter service. Be sure to use the included gasket between the end of the meter and the coupling.

**Connections**

MJE/MJHE and MJR/MJHR sensors are supplied with a color coded output cable (see diagrams below). Optional connectors can be ordered to plug directly into a Seametrics control or LMI metering pump.

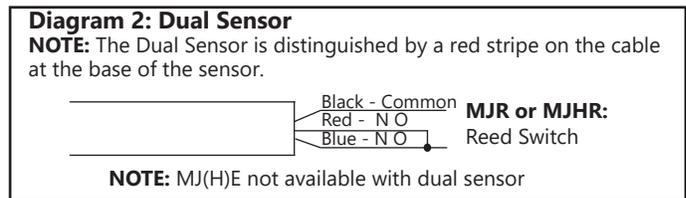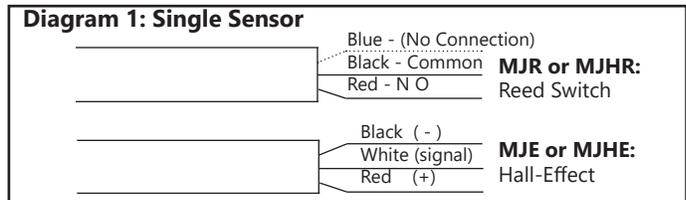

**To Distinguish Single Sensor From Dual:**

**Single:** (if new from factory) blue wire is cut back on cable end.  
**Dual:** A red stripe will be on cable near sensor.

**Note:** Dual sensor can be used as a single sensor also - use either the red OR the blue wire w/black. If using it as a dual sensor then connecting red and blue together will produce two pulses with every revolution of magnet.

**Pulse Output**

Both MJE/MJHE and MJR/MJHR sensors respond to a magnet that rotates on the face of the meter under the lens. The sensor turns on and off once each time the magnet passes under it. Sensors are designed for electronic control loads, and should not be used to switch power loads or line voltages. See maximum current and voltage ratings, under Specifications.

**Moving the Magnetic Pointer**



**NOTE!** When removing the large meter nut, Seametrics recommends using a 24" pipe wrench. Larger or smaller pipe wrenches may damage the nut on units!!

Remove meter top and lens, taking care not to lose the sealing ring. With fingers, lift the magnet pointer off its shaft and remove the plain pointer from the target dial. Reverse their positions and press them firmly into place. Securely seat the sealing ring and replace the lens, matching the tab on the lens to the notch on the meter to align the sensor with the magnetic pointer dial. Thread the meter top on and tighten.

**\*NOTE:** A special magnet (available from the factory) is required to achieve a rate of 4 pulses per gallon. It should be placed on the x0.1 dial, with non-magnetic pointers on the remaining dials. Otherwise, the procedure is the same.

**Setting Pulse Rates**

The pulse rate is determined by which sensor was ordered from the factory (single reed switch, dual reed switch, or single Hall-effect) and by the dial on which the magnet pointer is located. The pointer is set at the factory, but can be changed in the field as follows.

1. Find your desired pulse rate (Column 1)
2. Note the magnet pointer position (Column 2)
3. Move the magnet pointer to the appropriate dial position (see detailed instructions on next page)
4. Use the appropriate Connection Diagram (from Column 3) to wire the sensor to your remote device (using diagrams at right).

	Col. 1	Col. 2	Col. 3
Meter Size	Pulse Rate	Magnet Pointer Dial Position	Connection Diagram #
<b>3/4"</b>	*20 P/G	x0.01	2
	10 P/G	x0.01	1
	†4 P/G	x0.1	1
	*2 P/G	x0.1	2
	1 P/G	x0.1	1
	*5 G/P	x1	2
	10 G/P	x1	1
	*50 G/P	x10	2
	100 G/P	x10	1
<b>1"</b>	†4 P/G	x0.1	1
	*2 P/G	x0.1	2
	1P/G	x0.1	1
	*5 G/P	x1	2
	10 G/P	x1	1
	*50G.P	x10	2
	100 G/P	x10	1
<b>1-1/2"</b>	†4 P/G	x0.1	1
	*2 P/G	x0.1	2
	1 P/G	x0.1	1
	*5 G/P	x1	2
	10 G/P	x1	1
	*50 G/P	x10	2
	100 G/P	x10	1
<b>2"</b>	†4 P/G	x0.1	1
	*2 P/G	x0.1	2
	1 P/G	x0.1	1
	*5 G/P	x1	2
	10 G/P	x1	1
	*50 G/P	x10	2
	100 G/P	x10	1



\*These pulse rates available in MJR and MJHR dual reed switch meters only.  
 †This pulse rate available in MJR and MJHR single reed switch meters only.

**SAMPLE SET UP**

A 1" meter is shown with the magnet pointer set at the x10 dial, with a pulse rate of 100 Gallons per Pulse (that is, 10 increments on the x10 dial, or 10x10=100 Gal/Pulse).


**Reading Your Meter**

The Total Flow that has passed through your meter is read by starting at the top of the register with the Six-Digit Totalizer, and then reading clockwise around the small dials. In the example below, the Six-Digit Totalizer reads 13,800 (138 x 100), and the dials read 60 (6 x 10), 2 (2 x 1), and .4 (4 x .1) respectively. The Total Flow is 13,862.4 gallons.

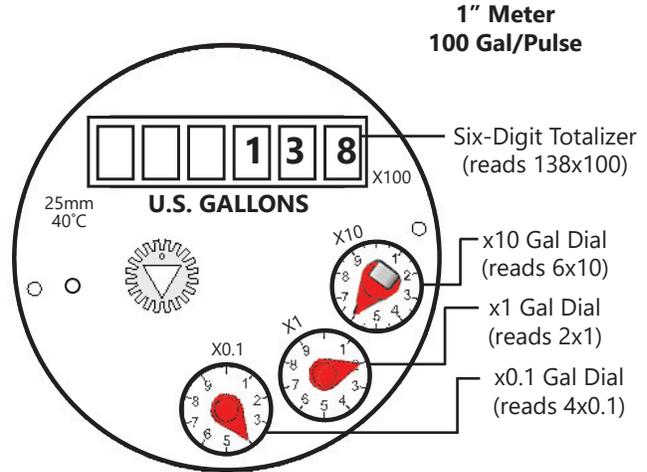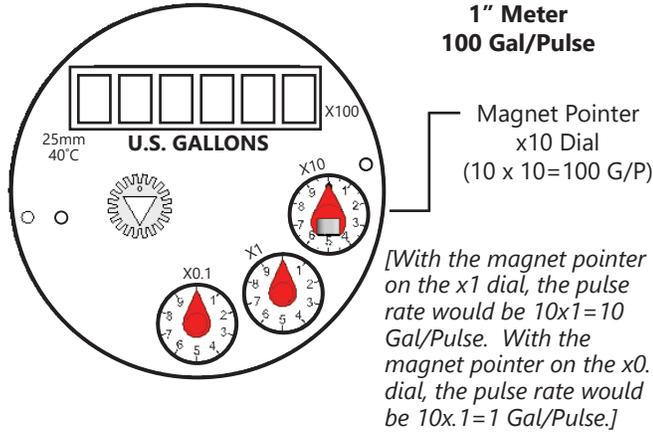


(NOTE: Disregard the **color** of the numbers on the totalizer when reading your total.) The "ones" digit is significant but the fact that it is red is not.

**Special Configurations**



The **3/4" meter** has a fourth dial, as shown above. The x0.01 dial is used for 20 P/G and 10 P/G rates. Note: The 3/4" meter has a 5 digit totalizer.



The **4 P/G rate** requires a special magnet, placed on the x0.1 dial, as shown above.

**MAINTENANCE**

Seametrics recommends all service to be performed by an authorized distributor or the factory to maintain the integrity of the protective tamper-proof wire-and-seal.

**Inlet Strainer**

Clean the strainer yearly, or as required, depending on water condition. Pull out the strainer or backflush the meter to loosen trapped particulates.

**Calibration**


Meters used for billing or billing exemption may be regulated by state or local authorities. New meters are factory-tested to meet the AWWA C-708 Multi-Jet Meter accuracy specification. Some states require retesting at various intervals, typically eight years for 3/4" meters, six for 1", and four for 1-1/2" and 2". Meters used for control should be tested every 5-10 years. Testing may be done by a local mobile meter service or in a private or municipal meter shop. Changes in calibration should be made at an authorized meter shop.

**Internal Parts Replacement**

All of the internal parts of an MJ-Series meter lift out as a unit, after the top has been unscrewed. The lens can then be removed and the internal assembly lifted out. If necessary, turn the meter upside down and tap one end lightly on a countertop to loosen the internals. The assembly can be separated by hand.

COLD WATER MODELS ONLY		¾"	1"
1	Lid and Hinge Pin Assembly	101068	101069
2	Lens Gasket Assembly	101071	101072
3	a Internal Assembly (gallons)	101073	101074
	b Internal Assembly (cubic feet)	101077	101078
4	Coupling Assembly (incl 2 sets)	101017	101018
5	Coupling Gasket Assembly (incl 2)	101081	101082
6	Lens	101004	101004
7	Sensor Screw	101045	101045
8	a Single Reed Switch Sensor (MJR)	103981	103981
	b Double Reed Switch Sensor (MJR)	103982	103982
	c Single Hall-Effect Sensor (MJE)	103983	103983
9	a Register (gallons)	100997	100998
	b Register (cubic feet)	101006	101007
	c Register (cubic meters)	103222-175	103222-100
	d Register (liters)	103333-075	103333-100
10	Internal Strainer	101016	101043
11	Tubular Strainer	101029	101030
12	Register Gasket	101013	101027

HOT WATER MODELS ONLY		¾"	1"
1	Lid and Hinge Pin Assembly	101354	101355
2	Lens Gasket Assembly	101332	101333
3	a Internal Assembly (gallons)	101350	101351
	b Internal Assembly (cubic feet)	101346	101347
4	Coupling Assembly (incl 2 sets)	101017	101018
5	Coupling Gasket Assembly (incl 2)	101081	101082
6	Lens	101004	101004
7	Sensor Screw	101045	101045
8	a Single Reed Switch Sensor (MJR)	103981	103981
	b Double Reed Switch Sensor (MJR)	103982	103982
	c Single Hall-Effect Sensor (MJE)	103983	103983
9	a Register (gallons)	101372	101373
	b Register (cubic feet)	101372	101373
	c Register (cubic meters)	103223-075	103223-100
	d Register (liters)	103334-075	103334-100
10	Internal Strainer	101379	101380
11	Tubular Strainer	101382	101383
12	Register Gasket	101013	101027

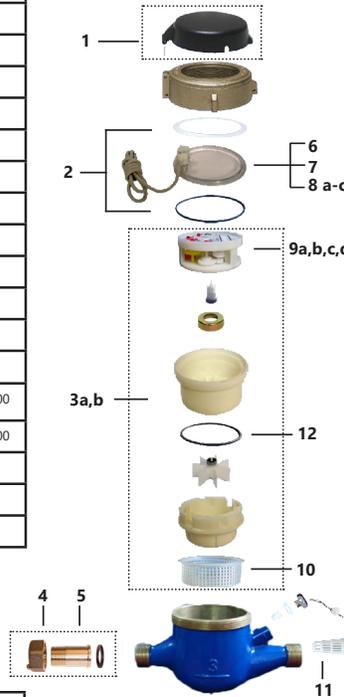

COLD WATER MODELS ONLY		1½"	2"
1	Lid and Hinge Pin Assembly	101070	101070
2	Lens Gasket Assembly	101085	101085
3	a Internal Assembly (gallons)	101075	101076
	b Internal Assembly (cubic feet)	101079	101080
4	Coupling Assembly (incl 2 sets)	101019	101020
5	Coupling Gasket Assembly (incl 2)	101083	101084
6	Lens	101004	101004
7	Sensor Screw	101045	101045
8	a Single Reed Switch Sensor (MJR)	103981	103981
	b Double Reed Switch Sensor (MJR)	103982	103982
	c Single Hall-Effect Sensor (MJE)	103983	103983
9	a Register (gallons)	100999	100999
	b Register (cubic feet)	101008	101009
	c Register (cubic meters)	103222-150	103222-200
	d Register (liters)	103333-150	103333-200
10	Internal Strainer	101044	101044
11	Tubular Strainer	101031	101032
12	Register Gasket	102228	102228

HOT WATER MODELS ONLY		1½"	2"
1	Lid and Hinge Pin Assembly	101356	101356
2	Lens Gasket Assembly	101334	101334
3	a Internal Assembly (gallons)	101352	101353
	b Internal Assembly (cubic feet)	101348	101349
4	Coupling Assembly (incl 2 sets)	101019	101020
5	Coupling Gasket Assembly (incl 2)	101083	101084
6	Lens	101004	101004
7	Sensor Screw	101045	101045
8	a Single Reed Switch Sensor (MJR)	103981	103981
	b Double Reed Switch Sensor (MJR)	103982	103982
	c Single Hall-Effect Sensor (MJE)	103983	103983
9	a Register (gallons)	101374	101375
	b Register (cubic feet)	101370	101371
	c Register (cubic meters)	103223-150	103223-200
	d Register (liters)	103223-150	103223-200
10	Internal Strainer	101381	101381
11	Tubular Strainer	101384	101385
12	Register Gasket	102228	102228

The limited warranty set forth below is given by Seametrics, with respect to Seametrics brand products purchased in the United States of America.

Seametrics warrants that products manufactured by Seametrics, when delivered to you in new condition in their original containers and properly installed, shall be free from defects in material and workmanship. **Seametrics products are warranted against defects for a minimum period of two (2) years from date of installation, unless otherwise specified, with proof of install date. If no proof of install date can be provided, warranty period will be two (2) years from date of shipment from Seametrics, as defined on Seametrics' invoice.** Seametrics' obligation under this warranty shall be limited to replacing or repairing the part or parts, or, at Seametrics' option, the products, which prove defective in material or workmanship. The following are the terms of Seametrics' limited warranty:

- a. Buyer must give Seametrics prompt notice of any defect or failure and satisfactory proof thereof.
- b. Any defective part or parts must be returned to Seametrics' factory or to an authorized service center for inspection.
- c. Buyer will prepay all freight charges to return any products to Seametrics' factory, or another repair facility, as designated by Seametrics.
- d. Defective products, or parts thereof, which are returned to Seametrics and proved to be defective upon inspection, will be repaired to factory specifications.
- e. Seametrics will deliver repaired products or replacements for defective products to the buyer (ground freight prepaid) to the destination provided in the original order.
- f. Products returned to Seametrics for which Seametrics provides replacement under this warranty shall become the property of Seametrics.
- g. This limited warranty covers all defects encountered in normal use of Seametrics products, and does not apply to the following cases:
  - i. Loss of or damage to Seametrics product due to abuse, mishandling, or improper packaging by buyer
  - ii. Failure to follow operating, maintenance, or environmental instructions prescribed in Seametrics' instruction manual
  - iii. Products not used for their intended purpose
  - iv. Alterations to the product, purposeful or accidental
  - v. Electrical current fluctuations
  - vi. Corrosion due to aggressive materials not approved for your specific product
  - vii. Mishandling, or misapplication of Seametrics products
  - viii. Products or parts that are typically consumed during normal operation
  - ix. Use of parts or supplies (other than those sold by Seametrics) which cause damage to the products, or cause abnormally frequent service calls or service problems
- h. A new warranty period will be established for repaired products, or products replaced during the original warranty period.
- i. In the event that equipment is altered or repaired by the buyer without prior written approval by Seametrics, all warranties are void. Damage caused by equipment or accessories not manufactured by Seametrics may void the product's warranty.
- j. SOFTWARE: The Seller grants the user a non-exclusive license to use Seametrics' software, according to the following limitations and conditions:
  - i. The user may install the software on one or more desktop or laptop computers.
  - ii. All title and intellectual rights to the software are owned by Seametrics.
  - iii. No copies may be made or distributed except as described above.
  - iv. The user may not modify or reverse-engineer the software.

THE FOREGOING WARRANTY IS IN LIEU OF ALL OTHER WARRANTIES, WHETHER ORAL, WRITTEN, EXPRESSED, IMPLIED OR STATUTORY. NO IMPLIED WARRANTY, INCLUDING ANY IMPLIED WARRANTY OF MERCHANTABILITY OR FITNESS FOR A PARTICULAR PURPOSE, APPLIED TO THE PRODUCTS AFTER THE APPLICABLE PERIOD OF THE EXPRESS LIMITED WARRANTY STATED ABOVE, AND NO OTHER EXPRESS WARRANTY OR GUARANTY, EXCEPT AS MENTIONED ABOVE, GIVEN BY ANY PERSON OR ENTITY WITH RESPECT TO THE PRODUCTS, SHALL BIND SEAMETRICS. SEAMETRICS SHALL NOT BE LIABLE FOR LOSS OF REVENUES, OR PROFITS, OR INCONVENIENCES, EXPENSE FOR SUBSTITUTE EQUIPMENT OR SERVICE, STORAGE CHARGES, LOSS OF DATA, OR ANY OTHER SPECIAL, INCIDENTAL, OR CONSEQUENTIAL DAMAGE CAUSED BY THE USE OR MISUSE OF, OR INABILITY TO USE THE PRODUCTS, REGARDLESS OF THE LEGAL THEORY ON WHICH THE CLAIM IS BASED, AND EVEN IF SEAMETRICS HAS BEEN ADVISED OF THE POSSIBILITY OF SUCH DAMAGES. IN NO EVENT SHALL RECOVERY OF ANY KIND AGAINST SEAMETRICS BE GREATER IN AMOUNT THAN THE PURCHASE PRICE OF THE PRODUCT SOLD BY SEAMETRICS AND CAUSING THE ALLEGED DAMAGE. WITHOUT LIMITING THE FOREGOING, YOU ASSUME ALL RISK OF LIABILITY FOR LOSS, DAMAGE, OR INJURY TO YOU AND YOUR PROPERTY AND TO OTHERS AND THEIR PROPERTY ARISING OUT OF USE OR MISUSE OF, OR INABILITY TO USE THE PRODUCTS NOT CAUSED DIRECTLY BY THE NEGLIGENCE OF SEAMETRICS.

SOME STATES DO NOT ALLOW LIMITATIONS ON THE DURATION OF AN IMPLIED WARRANTY, SO THE ABOVE LIMITATIONS MAY NOT APPLY TO YOU. SIMILARLY, SOME STATES DO NOT ALLOW THE EXCLUSION OR LIMITATIONS OF CONSEQUENTIAL DAMAGE, SO THE ABOVE LIMITATION OR EXCLUSION MAY NOT APPLY TO YOU. THIS LIMITED WARRANTY GIVES YOU SPECIFIC LEGAL RIGHTS; HOWEVER, YOU MAY ALSO HAVE OTHER RIGHTS WHICH MAY VARY FROM STATE TO STATE.

